

# Periodic acceptor excitation spectroscopy of single molecules

Sören Doose · Mike Heilemann · Xavier Michalet ·  
Shimon Weiss · Achillefs N. Kapanidis

Received: 22 November 2006 / Revised: 29 December 2006 / Accepted: 5 January 2007  
© EBSA 2007

**Abstract** Alternating-laser excitation (ALEX) spectroscopy has recently been added to the single-molecule spectroscopy toolkit. ALEX monitors interaction and stoichiometry of biomolecules, reports on biomolecular structure by measuring accurate Förster resonance energy transfer (FRET) efficiencies, and allows sorting of subpopulations on the basis of stoichiometry and FRET. Here, we demonstrate that a simple combination of one continuous-wave donor-excitation laser and one directly modulated acceptor-excitation laser (Periodic Acceptor eXcitation) is sufficient to recapitulate the capabilities of ALEX while minimizing the cost and complexity associated with use of modulation techniques.

**Keywords** Single-molecule fluorescence spectroscopy · Alternating-laser excitation (ALEX) · Förster resonance energy transfer (FRET) · Biomolecular interactions

## Introduction

Alternating-laser excitation (ALEX) spectroscopy combined with single-molecule Förster resonance energy transfer (smFRET) is a powerful tool for measuring distances and stoichiometry in individual molecules and for fluorescence-aided molecular sorting (Kapanidis et al. 2004, 2005a). ALEX was first demonstrated by alternating a green and a red laser at the microsecond time scale (Kapanidis et al. 2004). Fluorescence emission from spectrally distinct fluorophores was recorded at two distinct wavelength ranges and further distinguished by the excitation period (donor or acceptor) resulting in four separate photon-streams, which were used for calculations of FRET efficiency  $E$  and stoichiometry  $S$  for each detected fluorescence burst (due to the transit of a single molecule). A similar approach uses pulsed lasers with an interleaved pulse sequence, giving access to the fluorescence lifetime of each fluorophore (Kukolka et al. 2006; Laurence et al. 2005; Muller et al. 2005; Ruttinger et al. 2006). ALEX has been implemented at different time scales (nanosecond: ns-ALEX, microsecond:  $\mu$ s-ALEX, and millisecond: ms-ALEX), in wide-field and point-detection schemes, and on diffusing and immobilized molecules (Kapanidis et al. 2005a), and has been combined with fluorescence correlation spectroscopy (Doose et al. 2005; Muller et al. 2005). Recently, ALEX has been extended to three excitation lasers and three fluoro-

---

S. Doose · M. Heilemann · A. N. Kapanidis (✉)  
Clarendon Laboratory, Department of Physics and IRC  
in Bionanotechnology, Oxford University, Oxford, UK  
e-mail: a.kapanidis1@physics.ox.ac.uk

X. Michalet · S. Weiss  
Department of Chemistry and Biochemistry,  
University of California Los Angeles,  
607 Charles E. Young Drive East,  
Los Angeles, CA 90095-1569, USA

S. Weiss  
Department of Physiology,  
University of California Los Angeles,  
607 Charles E. Young Drive East,  
Los Angeles, CA 90095-1569, USA

S. Doose (✉)  
Applied Laser Physics and Laser Spectroscopy,  
University of Bielefeld, Bielefeld, Germany  
e-mail: sdoose@physik.uni-bielefeld.de

phores (3-color ALEX), a format that identifies populations containing up to three fluorophores, and obtains structural information by measuring up to three distances within single molecules (Lee et al. 2007).

The advantages of ALEX over smFRET (Deniz et al. 1999; Ha 2001) or coincidence methods (Li et al. 2003; Schwille et al. 1997) have been demonstrated by measuring accurate-FRET efficiencies (Lee et al. 2005), and by studying protein–DNA interactions (Kapanidis et al. 2004), gene transcription mechanisms (Kapanidis et al. 2005b), and biopolymer flexibility (Laurence et al. 2005). ALEX is also useful for FRET-based studies of biomolecular dynamics, since it distinguishes between true conformational changes and fluorophore photophysics [such as photoinduced on/off switching of carbocyanine dyes (Bates et al. 2005; Heilemann et al. 2005), typical FRET acceptors].

Currently, implementing  $\mu$ s-ALEX requires (i) adding electro-optical modulators and the associated polarization optics to each excitation laser used (Kapanidis et al. 2004), or (ii) coupling several laser wavelengths to an acousto-optical modulator (Nir et al. 2006), or (iii) using directly modulatable lasers, equipment that can be costly and represent an additional level of complexity. To simplify the use of  $\mu$ s-ALEX and thus increase its appeal to a wider scientific community, we describe here a simplified version of  $\mu$ s-ALEX, in which we dispense of modulating the donor-excitation laser, dubbed PAX for Periodic Acceptor eXcitation. Using doubly labeled DNA oligonucleotides as standards, we demonstrate that PAX is equivalent to conventional  $\mu$ s-ALEX in terms of extraction of the stoichiometry  $S$  and FRET efficiency  $E$  parameters.

## Materials and methods

### Sample preparation

Fluorescently labeled double-stranded DNA fragments with 35 bases were used as in Kapanidis et al. (2004). For single-molecule measurements, DNAs were diluted in 10 mM HEPES-HCl, pH 7.0, 500 mM NaCl, 100  $\mu$ g/ml BSA, 1 mM mercaptoethylamine, and 5% glycerol; the final concentration was  $\sim$ 100 pM.

### Optical setup


All experiments were performed on a home-built confocal microscope as illustrated in Fig. 1. Two laser beams [from a 532 nm green Nd:YAG laser (Samba, Cobolt AB), and a 638 nm red diode laser (Cube,

Coherent)] were coupled through a single-mode optical fiber (cut-off wavelength 488 nm, Thorlabs) into the optical path of an inverted microscope (IX71, Olympus). The red laser was modulated at 10 kHz using TTL signals. In PAX, the green laser was not modulated; in ALEX, the green laser was modulated using an electro-optical modulator (EOM) and a polarizer (P) (Kapanidis et al. 2004). Laser power was 300 and 80  $\mu$ W for the green and red laser, respectively, measured without modulation at the objective nosepiece. The beams were combined by a dichroic mirror (DM1) and focused through an oil-immersion objective (OBJ) (UPlanSApo 60 $\times$ , 1.35NA, Olympus) 30  $\mu$ m in solution. Fluorescence from diffusing molecules was collected through the objective, separated from excitation by a dichroic mirror (DM2), spatially filtered [using a 50  $\mu$ m pinhole (PH)], spectrally filtered [using a 585DF70 and a 650LP filter for the green and red channel, respectively, (F1) and (F2)] and detected using avalanche photodiodes [SPCM-AQR 14; Perkin Elmer, (APD1) and (APD2)]. Fluorescence bursts were identified and fluorescence contributions to the different channels computed. Background contributions were estimated from time traces of the four photon streams and subtracted from individual bursts for calculation of  $E$  and  $S$  values. Leakage and direct excitation were estimated from  $D$ -only and  $A$ -only samples, respectively. Only bursts with  $F_{A_{exc}}^{A_{em}} > 30$  (for ALEX) and  $\tilde{F}_{A_{exc}}^{A_{em}} > 30$  (for PAX) were included in analysis.  $E$  histograms were calculated from all bursts with  $S > 0.3$  to reject  $A$ -only bursts.  $S$  histograms were calculated from all detected bursts. The correction-detection factor  $\gamma$  was estimated to  $\gamma \approx 1$  from a linear plot of  $1/S$  as a function of  $E_{PR}$  (Eq. 6).

## Theory

Use of conventional ALEX results in four distinct photon-emission streams, corresponding to four distinct photon counts for every fluorescence burst (the observable from a single molecule diffusing through the confocal observation volume). Including crosstalk terms, the four photon counts for a single burst are  $F_{D_{exc}}^{D_{em}}$ ,  $F_{D_{exc}}^{A_{em}}$ ,  $F_{A_{exc}}^{A_{em}}$ , and  $F_{A_{exc}}^{D_{em}}$  [see Lee et al. (2005)]. For a typical FRET pair comprising a donor fluorophore ( $D$ ) and a red-shifted acceptor fluorophore ( $A$ ), the FRET signal is included in the  $F_{D_{exc}}^{A_{em}}$  photon count, which also includes crosstalk terms such as the  $D$ -emission into the  $A$ -detection channel ( $D$ -leakage,  $L_k$ ), and the  $A$ -emission due to  $A$ -direct-excitation at the  $D$ -excitation wavelength ( $A$ -direct-excitation,  $Dir$ ) (Lee et al. 2005). The crosstalk photons need to be calculated and sub-

**Fig. 1** Comparison of PAX and ALEX instrumentation and  $E$ - $S$  histogram. The confocal setup with either PAX or ALEX excitation path is illustrated as described in “Materials and methods”. Box  $E_{PR}$ - $S$  histograms recorded using PAX (left) and ALEX (right) for a 20 bp  $D$ - $A$  separation DNA

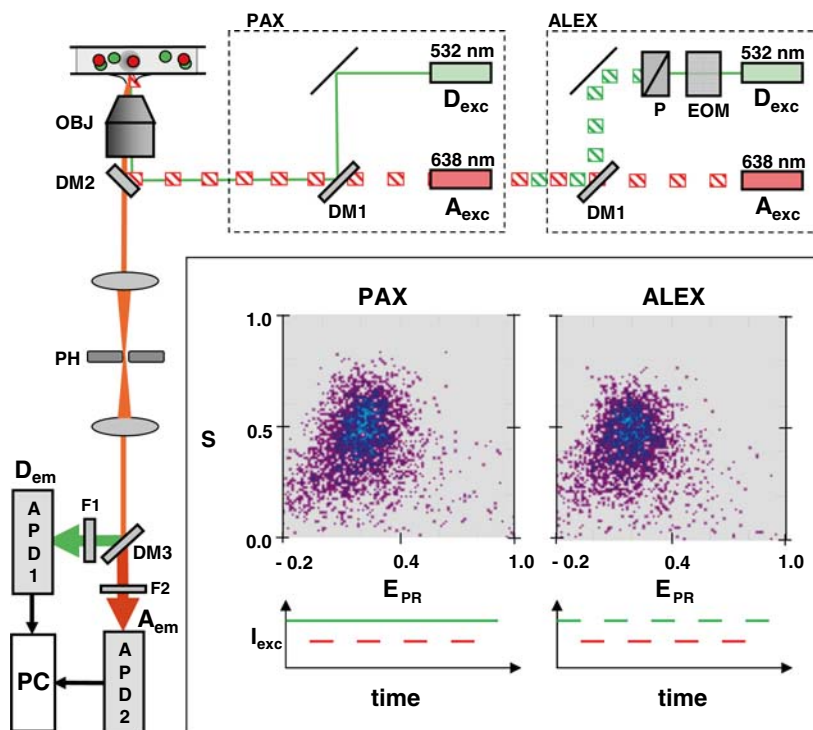

tracted for measuring accurate FRET from single molecules (Lee et al. 2005). The Lk crosstalk is defined as

$$Lk = l F_{D_{exc}}^{D_{em}} \tag{1}$$

where  $l$  is the  $D$ -leakage coefficient, determined using the ratio  $F_{D_{exc}}^{A_{em}}/F_{D_{exc}}^{D_{em}}$  as measured for  $D$ -only species. The Dir crosstalk is defined as  $Dir = d F_{A_{exc}}^{A_{em}}$ , where  $d$  is the  $A$ -direct-excitation coefficient, and determined using the ratio  $F_{D_{exc}}^{A_{em}}/F_{A_{exc}}^{A_{em}}$  as measured for  $A$ -only species. The FRET efficiency  $E$  for a single burst is defined as:

$$E = \frac{F^{FRET}}{\gamma F_{D_{exc}}^{D_{em}} + F^{FRET}}, \tag{2}$$

where  $F^{FRET} = F_{D_{exc}}^{A_{em}} - Lk - Dir$  and  $\gamma$  is a detection-correction factor that depends on the fluorophore quantum yields and the emission-channel detection efficiencies (Lee et al. 2005). The stoichiometry ratio  $S_\gamma$  for a single burst is defined as:

$$S_\gamma = \frac{\gamma F_{D_{exc}}^{D_{em}} + F^{FRET}}{\gamma F_{D_{exc}}^{D_{em}} + F^{FRET} + F_{A_{exc}}^{A_{em}}}. \tag{3}$$

Both  $E$  and  $S_\gamma$  are not directly observable in an experiment with unknown  $\gamma$ . We thus define the ratios  $E_{PR}$  and  $S$  as  $\gamma$ -independent experimental observables:

$$E_{PR} = \frac{F^{FRET}}{F_{D_{exc}}^{D_{em}} + F^{FRET}}, \tag{4}$$

$$S = \frac{F_{D_{exc}}^{D_{em}} + F^{FRET}}{F_{D_{exc}}^{D_{em}} + F^{FRET} + F_{A_{exc}}^{A_{em}}}, \tag{5}$$

where  $S$  is a function dependent of  $E_{PR}$ ; this relation is used to measure  $\gamma$  from experimental data (Lee et al. 2005):

$$1/S = 1 + \gamma\beta + \beta(1 - \gamma)E_{PR} = \Omega + \Sigma E_{PR}, \tag{6}$$

with  $\beta = \Omega + \Sigma - 1$  and  $\gamma = (\Omega - 1)/(\Omega + \Sigma - 1)$  ( $\Omega$  and  $\Sigma$  are the intercept and slope, respectively, of the linear relation in Eq. 6).

In PAX, the photon count  $F_{A_{exc}}^{A_{em}}$  is not experimentally observable (due to continuous  $D$ -excitation). However,  $F_{A_{exc}}^{A_{em}}$  can be calculated from the observed  $F_{D_{exc}+A_{exc}}^{A_{em}}$  (the photon count for  $A$ -emission under simultaneous  $D$ - and  $A$ -based excitation) and  $F_{D_{exc}}^{A_{em}}$ :

$$\tilde{F}_{A_{exc}}^{A_{em}} = F_{D_{exc}+A_{exc}}^{A_{em}} - F_{D_{exc}}^{A_{em}} \tag{7}$$

where  $\tilde{F}$  denotes a photon count measured indirectly; hereafter, the notation  $\tilde{X}$  will refer to variables that depend on  $\tilde{F}_{A_{exc}}^{A_{em}}$  (as in PAX) rather than on  $F_{A_{exc}}^{A_{em}}$  (as in ALEX). Combining Eq. 4, 5 and 7 we find an expression for  $E_{PR}$  and  $S$  based on PAX observables:

$$\tilde{E}_{PR} = \frac{\tilde{F}^{FRET}}{F_{D_{exc}}^{D_{em}} + \tilde{F}^{FRET}}, \tag{8}$$

$$\begin{aligned} \tilde{S} &= \frac{F_{D_{exc}}^{D_{em}} + \tilde{F}^{FRET}}{F_{D_{exc}}^{D_{em}} + \tilde{F}^{FRET} + F_{D_{exc}+A_{exc}}^{A_{em}} - F_{D_{exc}}^{A_{em}}} \\ &= \frac{F_{D_{exc}}^{D_{em}} + \tilde{F}^{FRET}}{F_{D_{exc}}^{D_{em}} + F_{D_{exc}+A_{exc}}^{A_{em}} - Lk - \tilde{Dir}}. \end{aligned} \tag{9}$$

To accurately evaluate Eqs. 8, 9, we need to determine Lk and  $\tilde{Dir}$  since  $\tilde{F}^{FRET} = F_{D_{exc}}^{A_{em}} - Lk - \tilde{Dir}$ . The leakage crosstalk is determined as described above, whereas to estimate the *A*-direct excitation, we use Eq. 7, replacing  $F_{A_{exc}}^{A_{em}}$  with  $\tilde{F}_{A_{exc}}^{A_{em}}$ :


$$\tilde{Dir} = d \tilde{F}_{A_{exc}}^{A_{em}} = d \left( F_{D_{exc}+A_{exc}}^{A_{em}} - F_{D_{exc}}^{A_{em}} \right), \tag{10}$$

where  $d = F_{D_{exc}}^{A_{em}} / \left( F_{D_{exc}+A_{exc}}^{A_{em}} - F_{D_{exc}}^{A_{em}} \right)$  is determined from *A*-only species.

## Results

To compare PAX and ALEX, we collected data from three samples of 100 pM solutions of 35 bp dsDNA with *D*-*A* separations of 10, 20, and 30 bp [as in Kapanidis et al. (2004)]. We collected data in ALEX mode and computed *E*-*S* histograms as described (Lee et al. 2005). We repeated the measurement using PAX by modulating only the red laser (using identical excitation powers, measured without modulation). After identification of fluorescence bursts and background subtraction, we constructed *E*-*S* histograms (Fig. 1) for *A*-containing bursts (selected using thresholds of  $F_{A_{exc}}^{A_{em}} > 30$  or  $\tilde{F}_{A_{exc}}^{A_{em}} > 30$  for ALEX and PAX, respectively; this filtering removes *D*-only molecules). Leakage and direct excitation were estimated from *D*-only and *A*-only samples, respectively, to be  $l \sim 8\%$  and  $d \sim 10\%$ . The detection-correction factor was  $\gamma \sim 1$  (Eq. 6).

**Fig. 2** Collapse of  $E_{PR}$ -*S* histograms for *D*-*A* labeled species on the  $E_{PR}$  (left) and *S* (right) axes. Each graph shows the  $E_{PR}$  or *S* distribution recorded using ALEX (black) and PAX (red) for DNA with *D*-*A* separation of 10 (a), 20 (b) and 30 (c) bp.  $E_{PR}$  histograms are calculated only for *D*-*A* molecules (using  $S > 0.3$  to reject *A*-only bursts). *S* histograms were calculated from all bursts

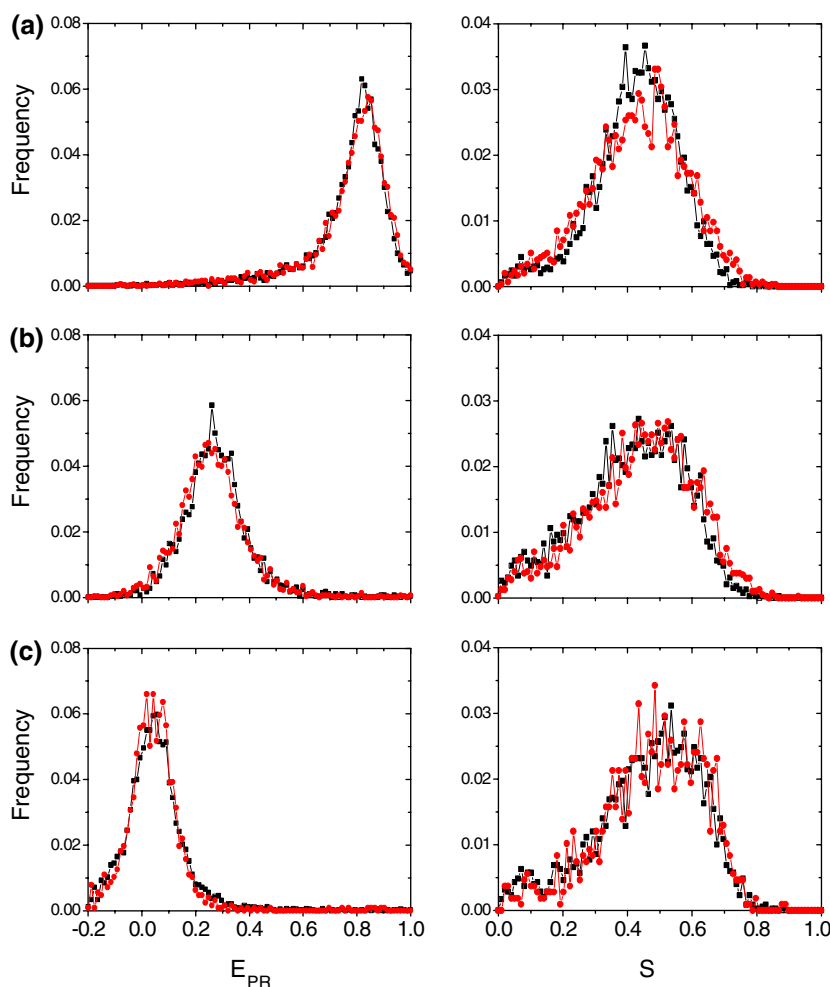

**Table 1** Means and standard deviations of  $E_{PR}$  and  $S$  distributions measured using ALEX and PAX

$D$ - $A$ separation (bp)	ALEX				PAX			
	$E_{PR}$		$S$		$E_{PR}$		$S$	
	Mean	STD	Mean	STD	Mean	STD	Mean	STD
10	0.773	0.144	0.428	0.130	0.776	0.151	0.433	0.147
20	0.275	0.123	0.414	0.160	0.261	0.127	0.441	0.164
30	0.052	0.117	0.462	0.163	0.046	0.107	0.477	0.157

Errors of the mean calculated from STD and the number of bursts for each measurement are smaller than  $5 \times 10^{-3}$  in all experiments

Our results establish that, for all DNAs, the 2D  $E_{PR}$ - $S$  histograms obtained using ALEX are essentially identical to the ones using PAX (Fig. 1). The excellent agreement is also clear after inspecting the collapse of  $E_{PR}$  and  $S$  histograms for all DNAs (Fig. 2; Table 1 for means and standard deviations), where it is shown that the distribution of  $E$  and  $S$  is identical within error [noise contributions to the  $E$  histogram have been discussed in detail by Antonik et al. (2006) and Nir et al. (2006)]. This demonstrates that a combination of a modulated red laser with a continuous green laser (PAX) is sufficient to discriminate between  $D$ -only,  $D$ - $A$ , and  $A$ -only molecules, and to extract FRET efficiencies identical to ALEX. The results also agree well with previously published experiments (Kapanidis et al. 2004; Lee et al. 2005) [note:  $E_{PR}$  differs from  $E_c$  in Kapanidis et al. (2004) in two ways: (i) we present mean values for  $E_{PR}$  whereas  $E_c$  represents the center of a fitted Gaussian distribution which slightly deviates at high  $E$ ; (ii) correction for  $A$ -direct excitation was not included in  $E_c$ ]. We conclude that PAX and ALEX are equivalent for determination of stoichiometry and FRET in a two-color sample.

## Conclusion

In conclusion, we have shown that ALEX can be implemented using a simplified format with a directly modulated red laser and a continuous-wave green laser. The mean values and standard deviations of the  $S$  and  $E$  distributions recovered using PAX are essentially identical to those measured by ALEX with two alternating lasers. Hence, the sorting and resolving capability of PAX is sufficient for separating  $D$ - $A$  labeled species with distinct FRET or distinct stoichiometry (e.g.,  $D$ -only or  $A$ -only species). Extension to more excitation lasers, as in 3-color ALEX (Lee et al. 2007), is straightforward and would result in the saving of one laser alternation. The technique can be applied at any time scale (nanosecond, microsecond, millisecond, etc) and geometry (diffusing molecules, immobi-

lized molecules, point detection or wide-field detection), as described in ref. (Kapanidis et al. 2005a). Overall, PAX enhances the ALEX methodology by substantially reducing the complexity and cost of instrumentation associated with ALEX.

**Acknowledgments** We thank N.K. Lee for providing DNA samples and L. LeReste for assistance. This work was funded by NIH grant GM069709-01 to S.W. and A.N.K., DOE grants 02ER63339 and 04ER63938 to S.W., and EPSRC grant EP/D058775, EU Marie Curie Fellowship MIRG-CT-2005-031079, and a UK Bionanotechnology IRC grant to A.N.K. M.H. was supported by a DAAD fellowship.

## References

- Antonik M, Felekyan S, Gaiduk A, Seidel CA (2006) Separating structural heterogeneities from stochastic variations in fluorescence resonance energy transfer distributions via photon distribution analysis. *J Phys Chem B* 110:6970–6978
- Bates M, Blosser TR, Zhuang X (2005) Short-range spectroscopic ruler based on a single-molecule optical switch. *Phys Rev Lett* 94:108101
- Deniz AA, Dahan M, Grunwell JR, Ha T, Faulhaber AE, Chemla DS, Weiss S, Schultz PG (1999) Single-pair fluorescence resonance energy transfer on freely diffusing molecules: observation of Förster distance dependence and subpopulations. *Proc Natl Acad Sci USA* 96:3670–3675
- Doose S, Tsay JM, Pinaud F, Weiss S (2005) Comparison of photophysical and colloidal properties of biocompatible semiconductor nanocrystals using fluorescence correlation spectroscopy. *Anal Chem* 77:2235–2242
- Ha T (2001) Single-molecule fluorescence resonance energy transfer. *Methods* 25:78–86
- Heilemann M, Margeat E, Kasper R, Sauer M, Tinnefeld P (2005) Carbocyanine dyes as efficient reversible single-molecule optical switch. *J Am Chem Soc* 127:3801–3806
- Kapanidis AN, Lee NK, Laurence TA, Doose S, Margeat E, Weiss S (2004) Fluorescence-aided molecule sorting: analysis of structure and interactions by alternating-laser excitation of single molecules. *Proc Natl Acad Sci USA* 101:8936–8941
- Kapanidis AN, Laurence TA, Lee NK, Margeat E, Kong X, Weiss S (2005a) Alternating-laser excitation of single molecules. *Acc Chem Res* 38:523–533
- Kapanidis AN, Margeat E, Laurence TA, Doose S, Ho SO, Mukhopadhyay J, Kortkhonja E, Mekler V, Ebright RH, Weiss S (2005b) Retention of transcription initiation factor [sigma]70 in transcription elongation: single-molecule analysis. *Mol Cell* 20:347–356

- Kukolka F, Muller BK, Paternoster S, Arndt A, Niemeyer CM, Bräuchle C, Lamb DC (2006) A single-molecule Förster resonance energy transfer analysis of fluorescent DNA-protein conjugates for nanobiotechnology. *Small* 2:1083–1089
- Laurence TA, Kong X, Jäger M, Weiss S (2005) Probing structural heterogeneities and fluctuations of nucleic acids and denatured proteins. *Proc Natl Acad Sci USA* 102:17348–17353
- Lee NK, Kapanidis AN, Wang Y, Michalet X, Mukhopadhyay J, Ebright RH, Weiss S (2005) Accurate FRET measurements within single diffusing biomolecules using alternating-laser excitation. *Biophys J* 88:2939–2953
- Lee NK, Kapanidis AN, Koh HR, Korlann Y, Ho SO, Kim Y, Gassman N, Kim SK, Weiss S (2007) Three-color alternating-laser excitation of single molecules: simultaneous monitoring of multiple interactions and distances. *Biophys J* 92:303–312
- Li H, Ying L, Green JJ, Balasubramanian S, Klenerman D (2003) Ultrasensitive coincidence fluorescence detection of single DNA molecules. *Anal Chem* 75:1664–1670
- Muller BK, Zaychikov E, Bräuchle C, Lamb DC (2005) Pulsed interleaved excitation. *Biophys J* 89:3508–3522
- Nir E, Michalet X, Hamadani K, Laurence TA, Neuhauser D, Kovchegov Y, Weiss S (2006) Shot-noise limited single-molecule FRET histogram: comparison between theory and experiments. *J Phys Chem B* 110:22103–22224
- Ruttinger S, Macdonald R, Kramer B, Koberling F, Roos M, Hildt E (2006) Accurate single-pair Förster resonant energy transfer through combination of pulsed interleaved excitation, time correlated single-photon counting, and fluorescence correlation spectroscopy. *J Biomed Optics* 11: 024012
- Schwille P, Meyer-Almes FJ, Rigler R (1997) Dual-color fluorescence cross-correlation spectroscopy for multicomponent diffusional analysis in solution. *Biophys J* 72:1878–1886